



ABSTRAX™ TECH

www.abstraxtech.com | info@abstraxlabs.com | 15550 Rockfield Blvd, Suite B120 | Irvine, CA 92618

Certificate of Analysis



Name: Do-Si-Dos
Matrix: Terpene Blend
Lot #: ABX0001155
Product #: ABXTB0051

CAS #:
Manufacture Date: 10/28/2019
Expiration Date: 10/28/2020
Overall Pass

Test	Specification	Result
Appearance	Colorless to yellow clear liquid	Pass

Volumetric glassware complies with Class A tolerance requirements of ASTM E 288 and NIST Circular 434; it is calibrated before first use and recalibrated regularly in accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Specific Gravity @ 25 °C	Specification	Result
Pass	0.85 - 0.89	0.87

Gas Chromatograph	Residual Solvent Analysis	Result
>90% purity	Pass	Pass

1, 2-Dichloroethane
Acetone
Acetonitrile
Benzene
Butane
Chloroform
Ethanol
Ethyl Acetate

Pass
Pass
Pass
Pass
Pass
Pass
Pass
Pass

Ethyl Ether
Ethylene Oxide
Heptane
Hexane
Isopropyl Alcohol
Methanol
Methylene Chloride
Naphtha

Pass
Pass
Pass
Pass
Pass
Pass
Pass
Pass


Pentane
Petroleum Ether
Propane
Trichloroethylene

Pass
Pass
Pass
Pass

Toluene
M-xylene
O-xylene
P-xylene

Pass
Pass
Pass
Pass

Instrument : GC-FID
Sample Name: DO SI DOS ABX0001155
Misc Info :
Vial Number: 56

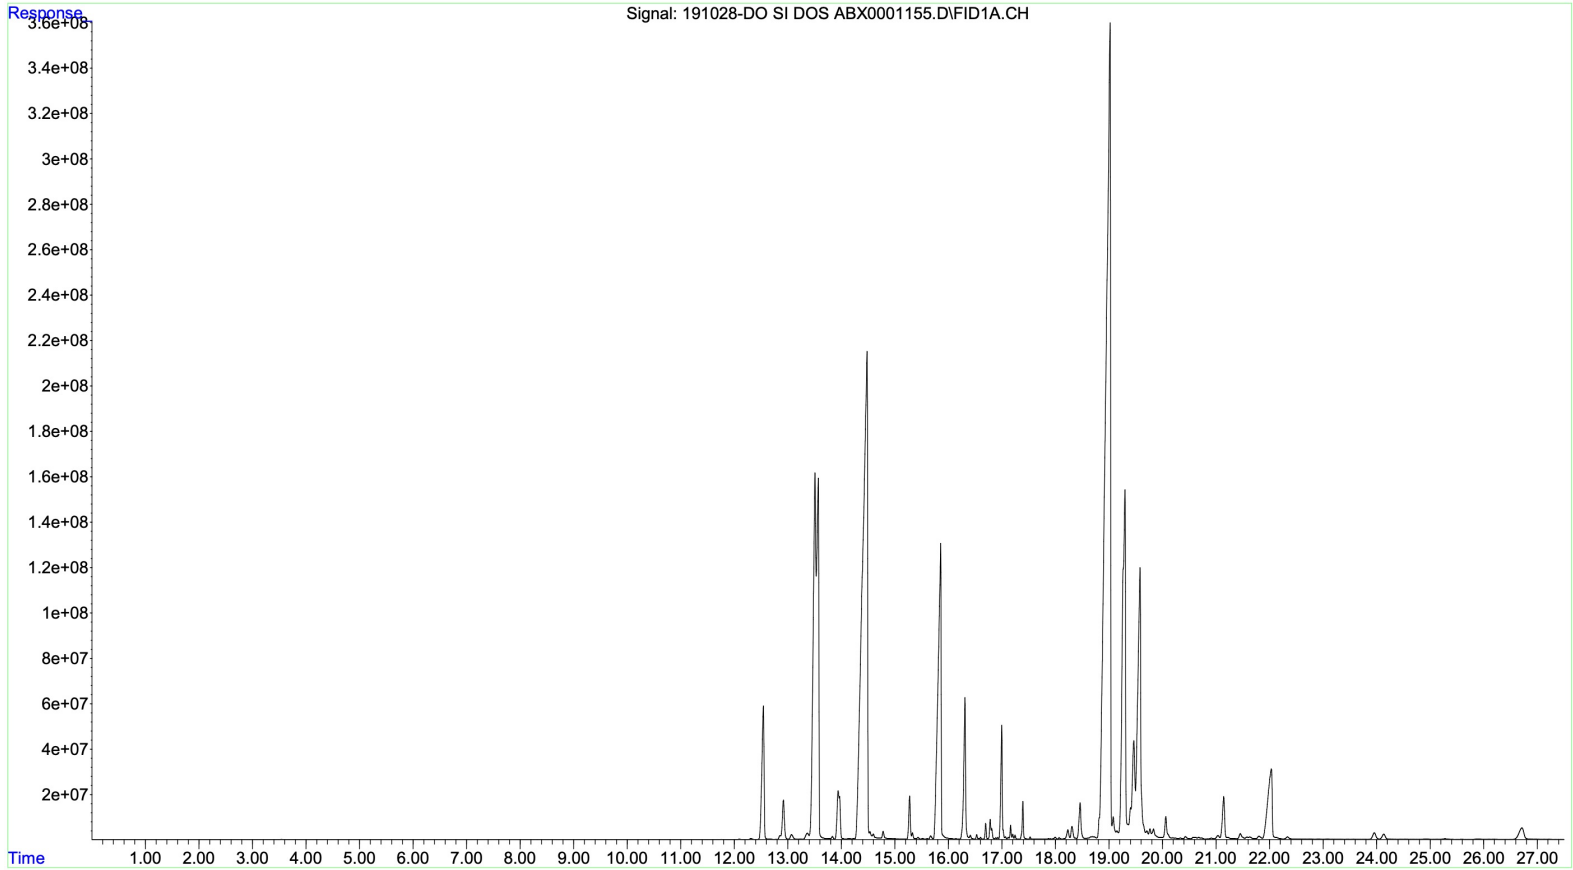

DATA REVIEWED AND APPROVED
BY:

Marcos Ojeda
Formulation Chemist

10/28/2019