

Certificate of Analysis

www.abstraxtech.com | info@abstraxlabs.com | 15550 Rockfield Blvd, Suite B120 | Irvine, CA 92618




Name: Matrix: Lot #: Product #:

Manufacture Date: Expiration Date: Overall Result:

Test	Specification Result			
Appearance				
Volumetric glassware complies with Class A tolerance re accordance with ASTM E 542 and NIST Procedure NBS	1	; it is calibrated before first use and recalibrated regularly eights certified traceable to the NIST national mass stan-	in	

accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Specific Gravity @ 25 °C	Speci	fication		Resu		
Gas Chromatograph	Residual Solvent Analysis			Water Activity (A _W)		
1,2-Dichloroethane		Ethyl Ether				
Acetone		Ethylene Oxide				
Acetonitrile		Heptane				
Benzene		Hexane				
Butane		Isopropyl Alcohol				
Chloroform		Methanol				
Ethanol		Methylene Chloride	9			
Ethyl Acetate		Pentane				

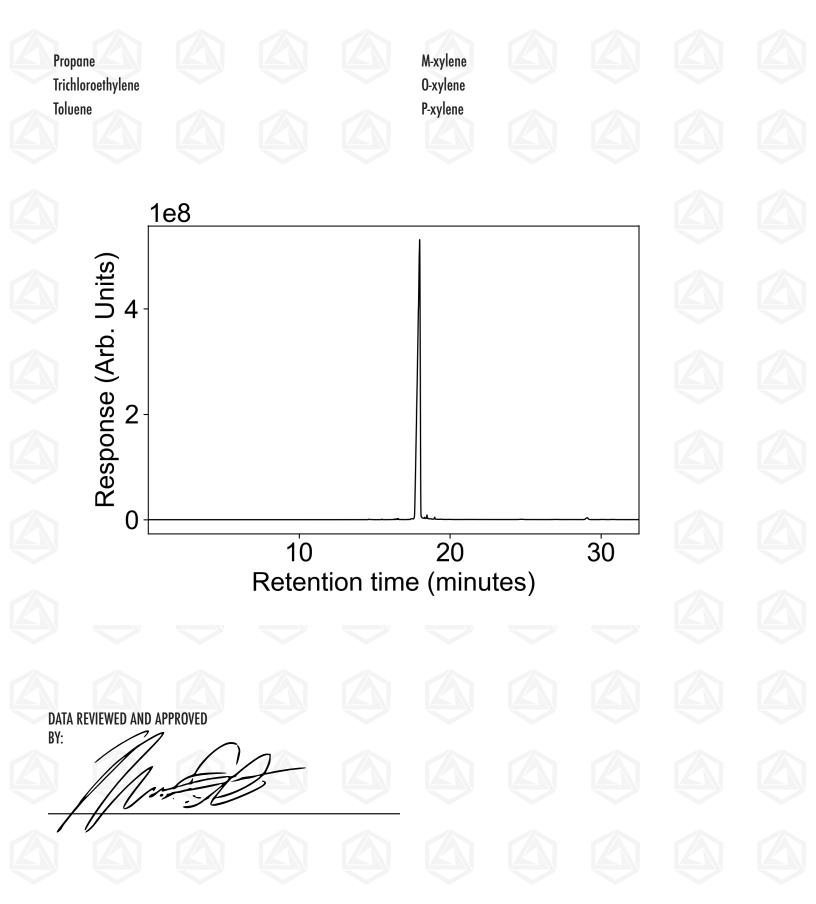

This Certificate of Analysis is accurate to the best of our knowledge. However, the customer is responsible for performing its own assessment to ensure that the material is suitable for its intended applications, including compliance with all pertinent legal requirements. The expected shelf life is calculated from the original manufacture date and is based on unopened containers stored under proper conditions. Once containers have been opened, maintaining minimal headspace and storing under appropriate conditions will aid in preserving the product's integrity.