




ABSTRAX™

TECH

www.abstraxtech.com | info@abstraxlabs.com | 15550 Rockfield Blvd, Suite B120 | Irvine, CA 92618

Certificate of Analysis



Name:
Matrix:
Lot #:
Product #:

CAS #:
Manufacture Date:
Expiration Date:
Overall Result:

Test	Specification	Result
Appearance		

Volumetric glassware complies with Class A tolerance requirements of ASTM E 288 and NIST Circular 434; it is calibrated before first use and recalibrated regularly in accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Specific Gravity @ 25 °C	Specification	Result


Gas Chromatograph	Residual Solvent Analysis	Result

Acetone
Acetonitrile
Benzene
Butane
Ethanol
Ethyl Acetate
Ethyl Ether
Heptane

Hexane
Isopropyl Alcohol
Methanol
Methylene Chloride
Pentane
Propane
Toluene
M-xylene

O-xylene
P-xylene

Instrument : GC-FID
Sample Name: SAP P30
Misc Info :
Vial Number: 10

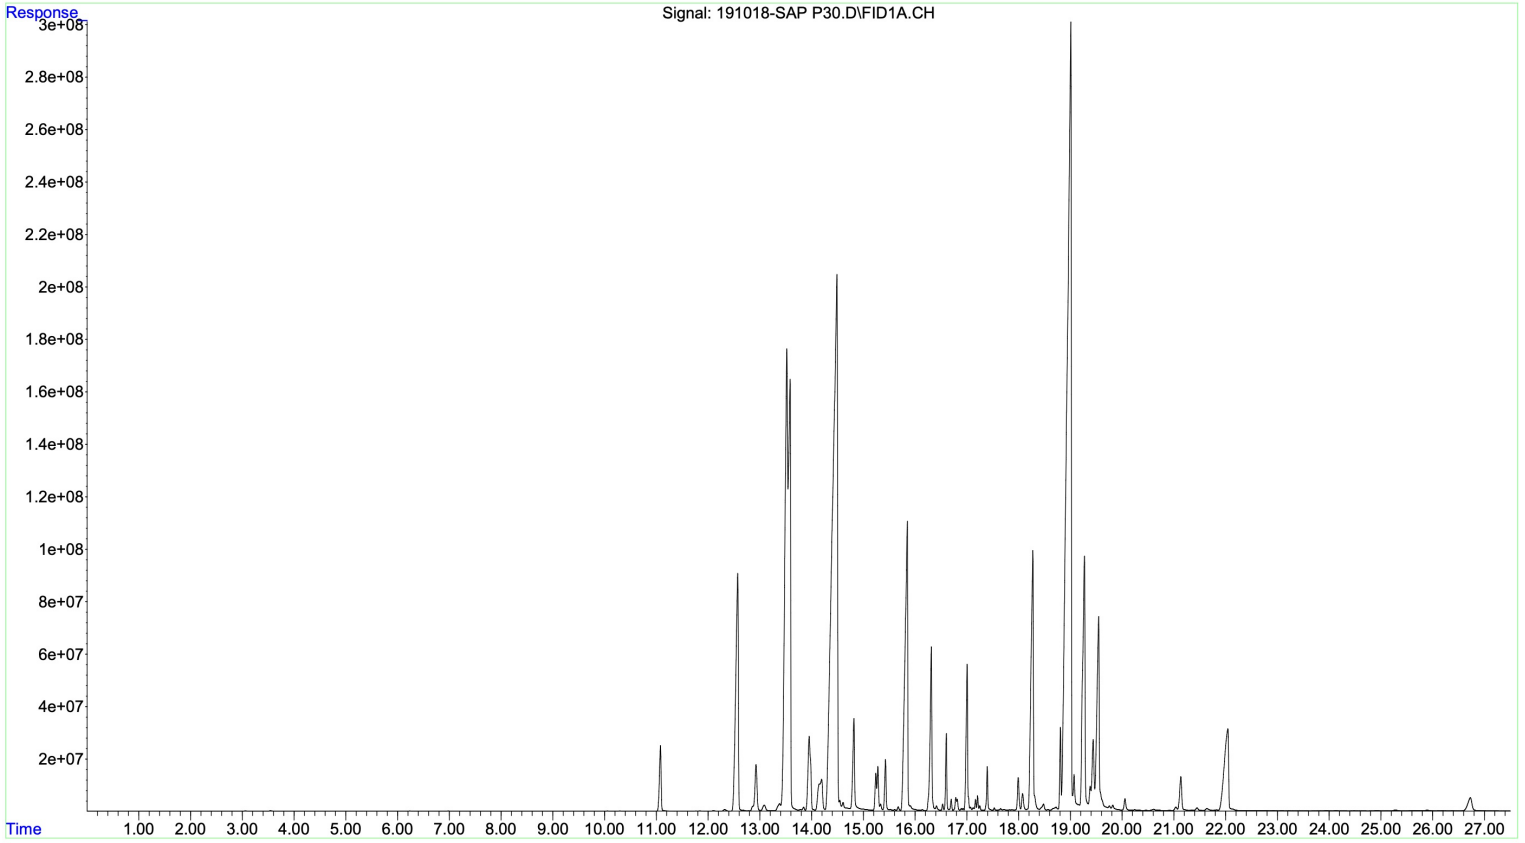

DATA REVIEWED AND APPROVED
BY:

SAP