


## Toilet-to-Tub Sliding Transfer Bench - Parts Reference Sheet

## Assembly Instruction Sheet



1. Take the leg frame with the handlebar (Part A), and lay it flat on the ground.
2. Determine which direction you would like the seat to face in your bathtub. The leg frame with the handlebar (Part A) will be the side that goes inside the bathtub.
3. There are two sliding rails (Part C): one rail has 4 brass push buttons (front rail), and the other rail has 2 push buttons (rear rail).
4. If you prefer to sit facing left (if looking at the tub from outside), take the rail with 4 push buttons (front rail), and insert it into tube X (or insert it into tube Y if you want to sit facing right). Make sure the two smaller push buttons face forwards (the smaller push buttons are for the sliding rail locking mechanisms). Make sure the larger button snaps firmly into the leg frame.
5. Insert the rear sliding rail into the other side of the leg frame (Part A), making sure the button snaps firmly into place.

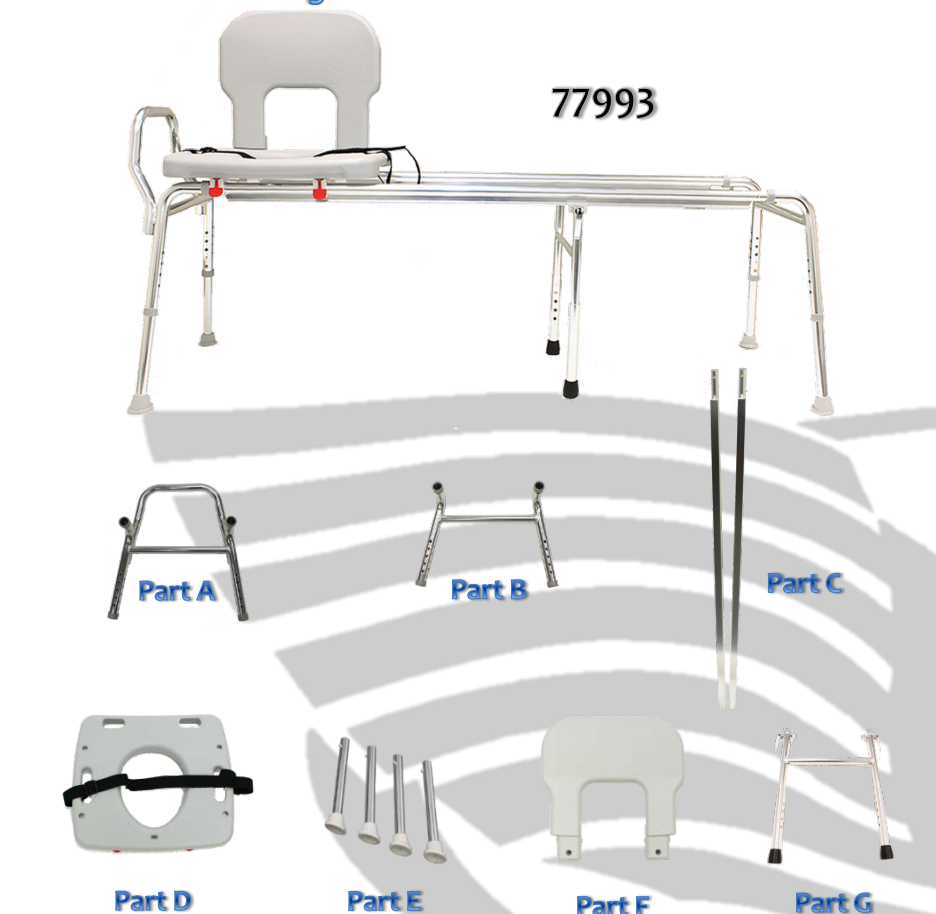


6. Take the seat with the attached sliding rings (Part D), and align the sliding rings with the rails, so that the locking side of the seat (the side with the red tabs) is on the same rail as the 4 brass push buttons. Insert both sliding rails into the sliding rings under the seat. Push in push buttons to slide the seat easily onto the rails.



7. Take the other leg frame (Part B), and insert the sliding rails into it. Make sure the brass buttons snap firmly into place.



8. Place leg-support (Part G) along the under-side of rails. Ensure the black rubber platforms at the top of the leg-support are flush with the flat underside of the sliding rails. If necessary, loosen thumb-nut to widen the top L-plate of the clamp to install. Make sure top L-plate is positioned above the flat part of the rail.

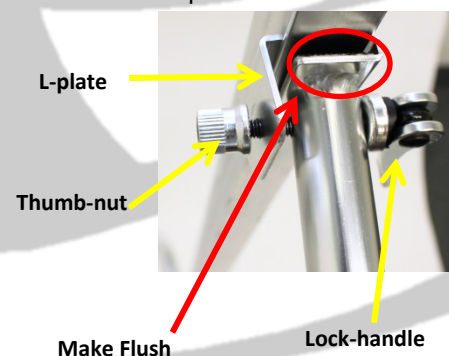

9. Position the leg-support (Part G) at mid-point along the sliding rails before tightening. With the clamp lock-handle open (perpendicular to the legs), tighten the thumb-nut. Then flip the lock-handle down to lock the clamp.



**CAUTION:** Do not over-tighten.

The top L-plate should sit flat with the top of the flat part of the sliding rail. The lock-handle will bounce back to perpendicular if over-tightened.



10. Take the 4 legs (Part E), and insert them into the leg frames. Set bench height by using same button-hole location for each leg. Make sure the buttons snap firmly into place. For your safety, adjust the rubber tips on the legs by turning them outward for maximum floor contact. Sit the bench up on the legs.

11. Insert the backrest (Part F) into the two oblong holes on top of the seat towards the rear of the seat. Push backrest down firmly into seat until it snaps into place.



Thank you for purchasing an Eagle Health Supplies product!

Helpful instructional assembly videos available at [www.EagleHealth.com](http://www.EagleHealth.com).

**If any push button/pin does not completely snap into place while assembling, or if you feel the bench is not secure, please do not use the bench, and notify your Authorized Dealer immediately.**

*To register your product for the Limited One-Year Warranty, please complete and return the included Warranty Card, or register online at [www.EagleHealth.com](http://www.EagleHealth.com).*

## Tips for Care and Use


### Locking Mechanism

Lock the seat into place by making sure the slide ring snaps firmly onto the brass push button at the end of the sliding rail (shown below). Release the locking mechanism by pressing down on the red tab of the locked slide ring.

**UNLOCKED**



**LOCKED**



### Middle Leg-Support

Adjust the leg height so the legs are barely off the ground (about 1/8" to 1/4"). Make sure the buttons snap firmly into place.

### Rubber Tips

Be sure the rubber tips are turned outward for maximum floor contact and stability.

### Cleaning

Rinse off the bench with warm water after each use to prevent dirt, soap scum, and mineral deposits from forming which could affect proper operation. We recommend regularly cleaning the seat and back with a soft cloth, warm water and mild soap, or with a soft cloth and any non-bleach cleaner.

### Maintenance

Built up soap scum, mineral deposits, or watermarks may cause the brass push buttons/pins to stick or may cause the seat to not slide smoothly along the rails. To help, spray lubricant, such as WD-40, on the brass push buttons/pins to loosen the buttons/pins, or along the sliding rails to maintain a smooth slide.



**EAGLE HEALTH SUPPLIES INC.**  
[www.eaglehealth.com](http://www.eaglehealth.com)

# Instruction Pamphlet

**For Toilet-to-Tub Sliding Transfer Benches**

**77963 / 77983 / 77993 / 77903 / 77913**

**For Your Comfort. For Your Safety.**

**For Your Independence. For YOU.**